


LIFE SOURCE[®]

DIGITAL THERMOMETER

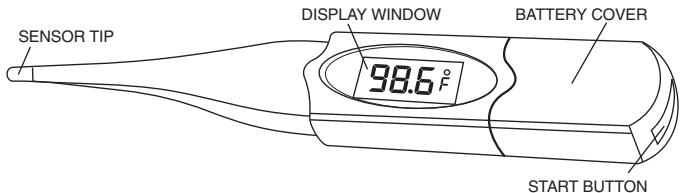


Instruction Guide – MODEL DT-607

Congratulations on your purchase of the LifeSource[®] Digital Thermometer. Please read the instructions carefully to ensure accurate temperatures and safe operation. When used properly, this high quality product will give you years of accurate, dependable service.

SAFETY INFORMATION

- High, prolonged fever requires medical attention (over 100.0°F or 37.8°C) for young children. In case of high readings, please contact your physician.
- Do not allow children to take their temperature unattended.
- Read the enclosed instructions carefully to ensure accurate temperature readings. Temperature readings are affected by many factors including exercise, drinking hot or cold beverages prior to taking, and technique.
- Do not allow children to walk or run during temperature taking. The rigid probe could present a hazard.
- Oral, underarm, and rectal temperatures vary by approximately 1°F (0.5°C).

SPECIAL PRODUCT FEATURES

- Reads temperature in Fahrenheit or Celsius.
- Memory feature: automatic recall of last temperature reading.
- Beeps when peak temperature is reached.
- Auto-Off in approximately 9 minutes.
- Thermometer is water resistant, but not 100% waterproof. Do not submerge unit in any liquid.
- Long-life, replaceable battery (approximately 3,000 temperatures).
- Low Battery Indicator “”.
- Oral, Rectal or Underarm use.

HOW TO CARE FOR THIS PRODUCT

- The thermometer should be cleaned after every use even when probe covers are used.
- Clean the thermometer tip and probe using isopropyl alcohol or soap and water. Do not boil the thermometer. Do not submerge the thermometer in any liquid.
- Store the unit in the protective case while not in use.
- Do not store or keep in direct sunlight, or in high temperatures.
- Do not open the thermometer except to replace the battery.
- Do not drop the thermometer, as this may break the unit.
- Do not attempt to disassemble the unit except to replace the battery.

WHAT IS A “NORMAL” TEMPERATURE?

Temperature readings vary among individuals. A normal temperature refers to each individual's average temperature while they are well. Normal average temperatures range from 97°F/36.1°C to 100°F/37.7°C when taken orally. A rectal temperature is considered your real or “core” body temperature. A rectal temperature is 1°F/0.5°C higher than an oral reading and an underarm temperature is 1°F/0.5°C lower than an oral reading.


HOW TO TAKE TEMPERATURE

1. Select oral, underarm or rectal as your measurement site (see following instructions).
2. Push the START button located at the top of the thermometer. The thermometer will beep and the display will show all symbols.. This is a function check indicating the unit is working properly. If a previous reading is stored in memory, the thermometer will display the last temperature for two seconds. The flashing symbol °F (or °C) will appear with the “L” or “H” symbol indicating that the thermometer is ready for measurement. Begin measurement.
3. When the °F (or °C) symbol stops flashing and the thermometer emits eight beeps, the temperature measurement is complete.
4. Read and record the temperature and time for reference. The reading will automatically be stored in the memory until another reading is taken or the batteries are removed from the thermometer.
5. Push the START button to turn the unit off. If you do not turn the unit off, it will shut off automatically in approximately 9 minutes.

NOTE: If the measured temperature is higher than 99.5°F (37.5°C), the fever alarm will beep quickly for about four seconds.


ORAL USE

- Do not drink hot or cold fluids, exercise, smoke or perform other activities that raise or lower temperature. The mouth should remain closed up to 5 minutes before attempting a reading.
- Place the probe tip well under the tongue in locations as indicated by the “✓” (see diagram). Instruct children not to bite down on the probe.
- The approximate measurement time is 60 seconds. Opening the mouth or improper placement of the probe tip may result in a longer time for a reading.



UNDERARM (AUXILIARY) USE

- From a medical point of view, this method will always give an inaccurate reading and should not be used if a precise measurement is required.
- Wipe underarm with a dry towel.
- Place probe tip in armpit and bring arm down against the body. The measuring sensor should be pointing upward parallel to the arm.
- The approximate measurement time may be 5 minutes or longer depending on the placement of the probe and closure of the arm against the body.



RECTAL USE

- Commonly used for babies, young children or when it is difficult to take an oral or underarm temperature.
- After placing the probe cover on the thermometer, lubricate with a water-soluble jelly such as K-Y Jelly®.
- Gently insert the probe tip no more than 1/2 inch or 1.3 cm into the rectum. Do not force the tip into the rectum if resistance is encountered.
- Wash the thermometer as recommended.
- Approximate measurement time is 60 seconds.
- Once used rectally, the thermometer should not be used orally for sanitary reasons.

CLEANING INSTRUCTIONS


Wash the area extending about 2" from the tip with warm, soapy water after each use and dry thoroughly.

OR

Wipe the area extending about 2" from the tip with 70% isopropyl alcohol after each use.

NOTE: Do not submerge the thermometer in any liquid.

CHANGING THE BATTERY

When the “” appears and blinks, the battery needs to be replaced. Make sure you use the same type of battery and proceed as follows: Remove battery compartment lid. Use a non metal probe to remove battery. Insert new equivalent battery type (1.55V or LR41). Ensure battery is correctly positioned with the “+” facing up. Carefully replace the battery compartment lid. Properly dispose of the battery, keeping it from small children and heat.

SWITCHING BETWEEN FAHRENHEIT & CELSIUS

1. Press START button.
2. Wait until “L” symbol appears and °F (°C) starts flashing.
3. Press and hold START button until °F (°C) symbol flashes five times.
4. Release the START button. The thermometer is now changed to °C (°F).
5. The thermometer is now ready for measurement.

SPECIFICATIONS

RANGE	32.0°C - 44.0°C 90.0°F - 110.0°F
ACCURACY MEASUREMENT RANGE	± 0.3°F less than 95.0°F ± 0.2°F from 95.0°F to 107.6°F ± 0.3°F from 107.6°F to 109.4°F ± 0.2°C less than 35.0°C ± 0.1°C from 35.0°C to 42.0°C ± 0.2°C from 42.0°C to 43.0°C
DISPLAY	0.1°F (0.1°C)
BATTERY	One 1.55V button size battery (LR41 type or equivalent)
POWER CONSUMPTION	Less than or equal to 0.09mW
BATTERY LIFE	Approximately 200 hours of continuous operation
DIMENSIONS	5.1 x 0.6 x 0.3" (13.2 x 1.65 x 0.93 cm)
WEIGHT	Approximately 13 grams including battery

PRECAUTIONS

- Do not drop unit or subject to shock.
- Do not boil the probe. Clean the probe with isopropyl alcohol.
- Do not use solvents or thinners on the unit.
- Do not store the unit in direct sunlight or at high temperature.
- Do not attempt to disassemble the unit except to replace the battery.

WARRANTY

A&D Medical warrants to the first retail purchaser that this digital thermometer is free from defects in material and workmanship for the lifetime of the original owner. This warranty does not cover batteries or damage resulting from improper handling or use. To obtain replacement product, please return the product, freight and insurance prepaid, together with proof of purchase and applicable shipping costs to LifeSource at the address below. Call the toll-free LifeSource Health Line at 1-888-726-9966 for shipping costs and further information. At LifeSource's option, the product will be replaced with a new or refurbished product of equal value. THE WARRANTY AND REMEDY PROVIDED ABOVE ARE EXCLUSIVE AND IN LIEU OF ALL OTHER EXPRESS WARRANTIES.

A&D Medical
A division of A&D Engineering
1555 McCandless Drive
Milpitas, CA 95035
Toll-free LifeSource Health Line 1-888-726-9966
www.LifeSourceOnline.com

K-Y Jelly® is a registered trademark of Johnson & Johnson.
LifeSource® is a registered trademark of A&D Medical.
© 2006 A&D Medical.
Made in China